

1/6

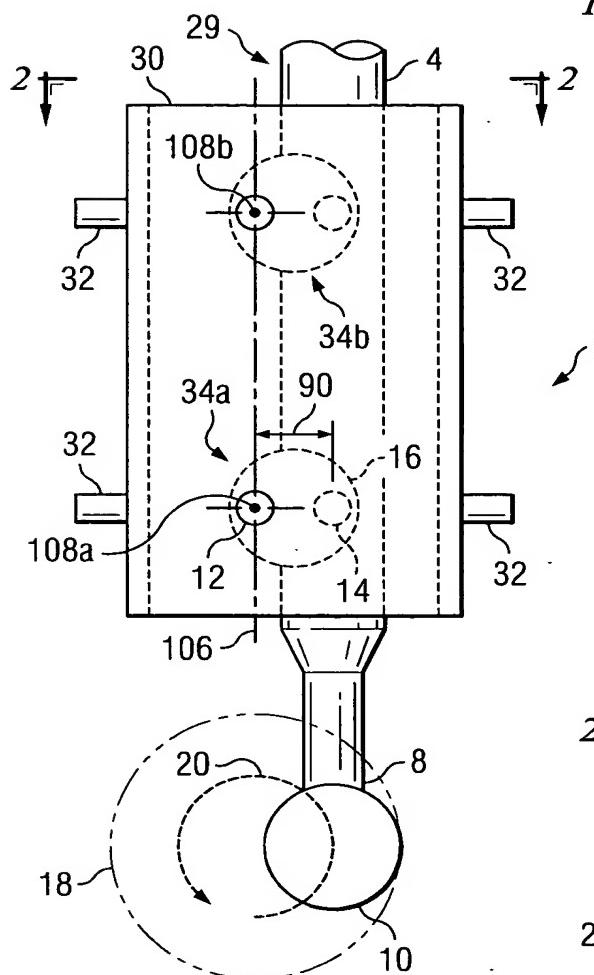


Fig. 1A

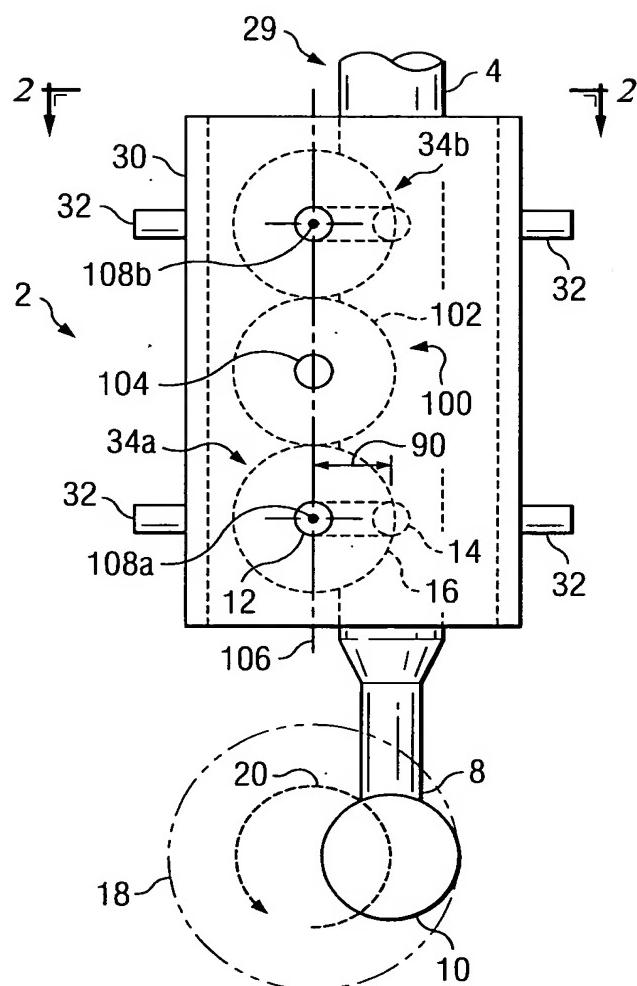


Fig. 1B

2/6

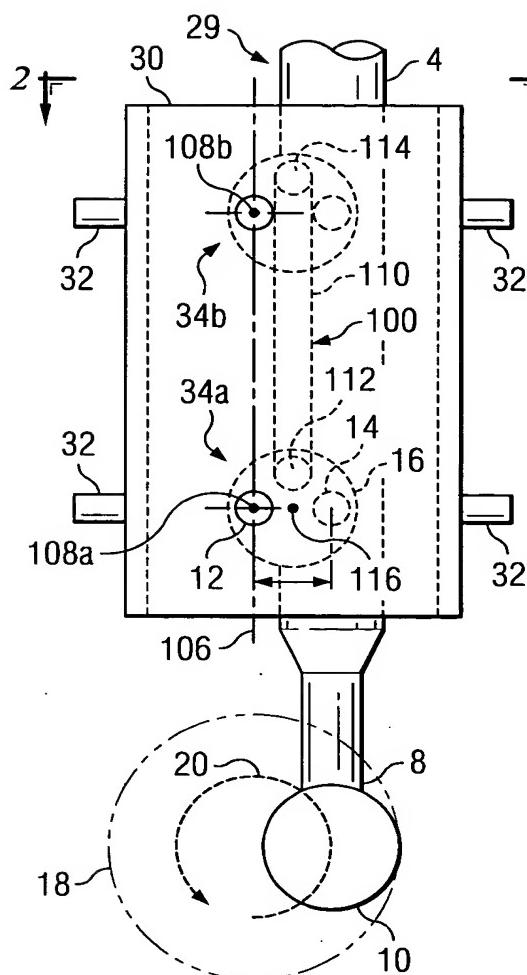


Fig. 1C

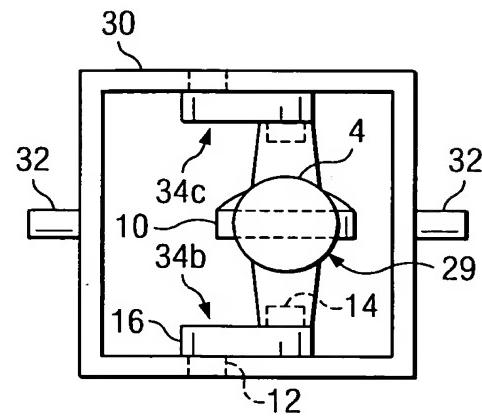


Fig. 2

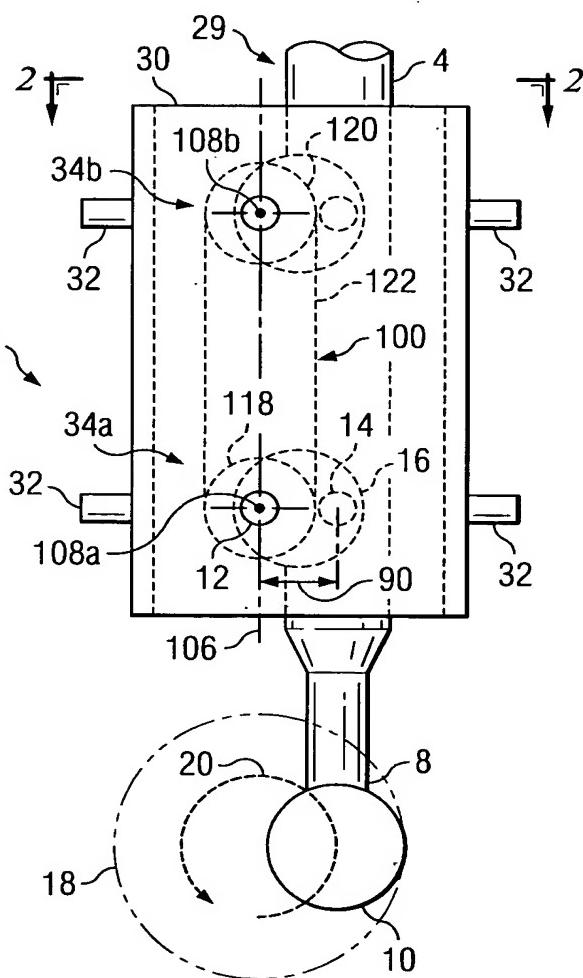


Fig. 1D

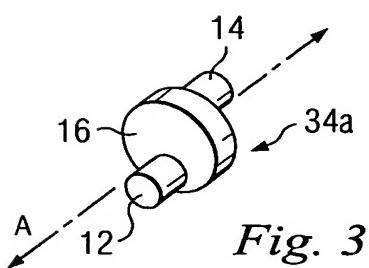
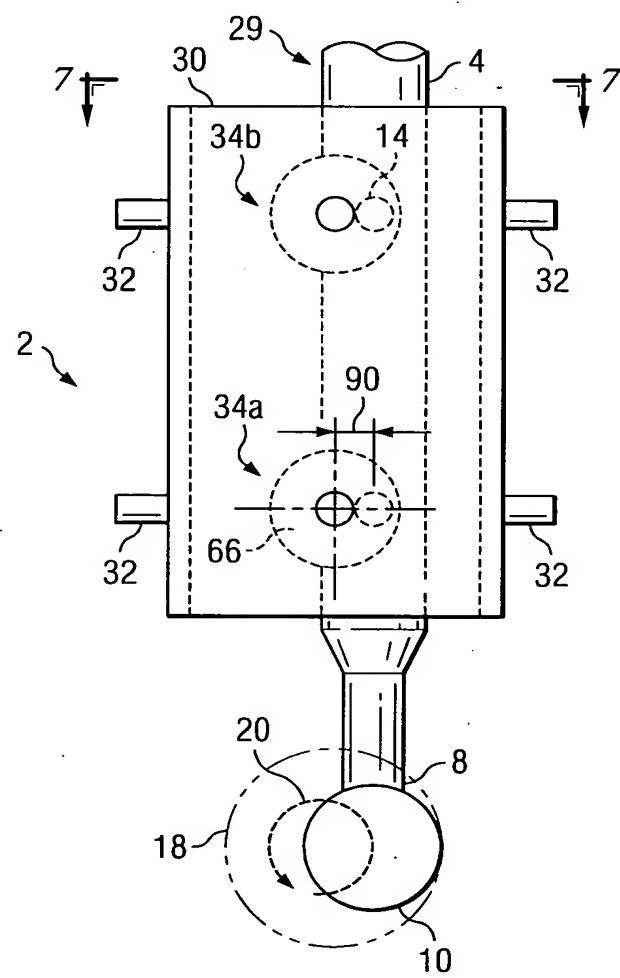
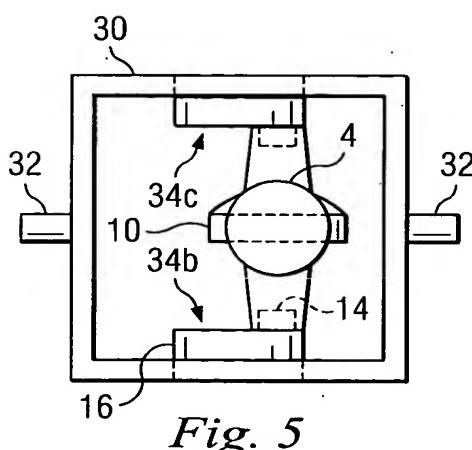
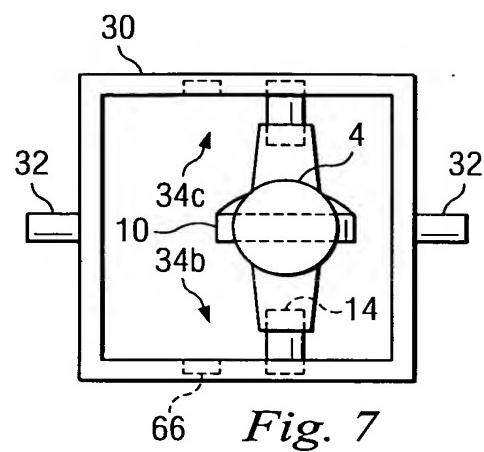
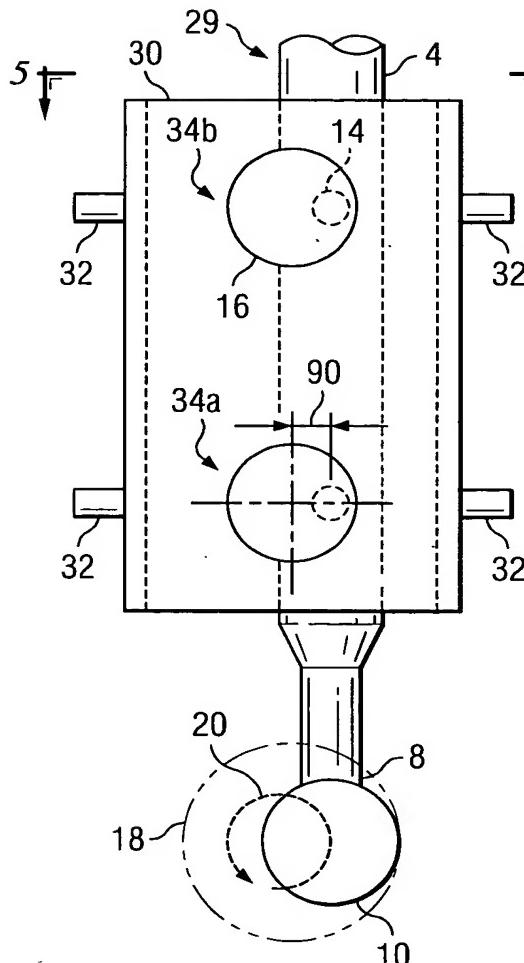


Fig. 3

3/6



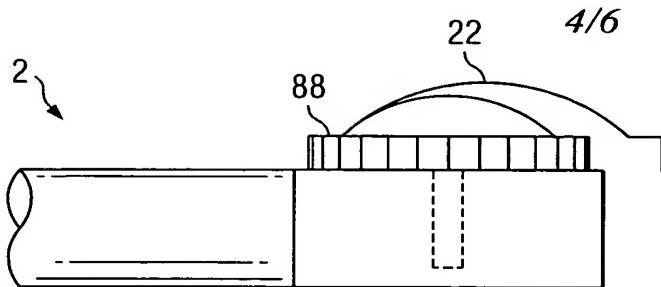


Fig. 8A

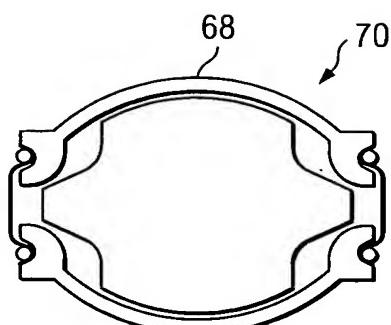


Fig. 8B

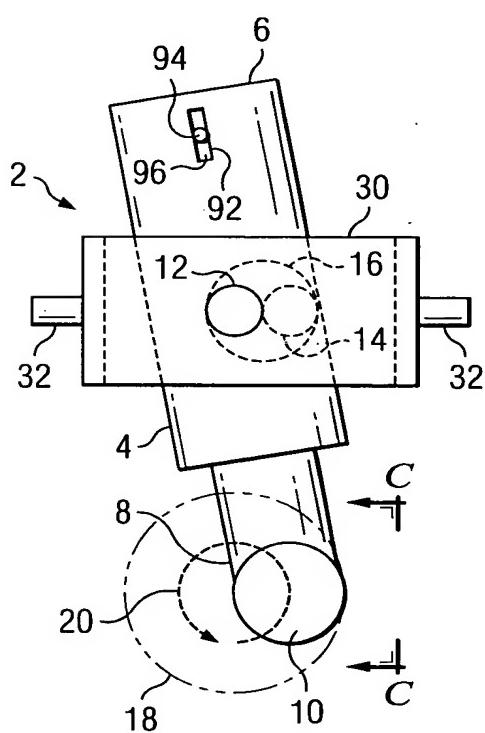


Fig. 9A

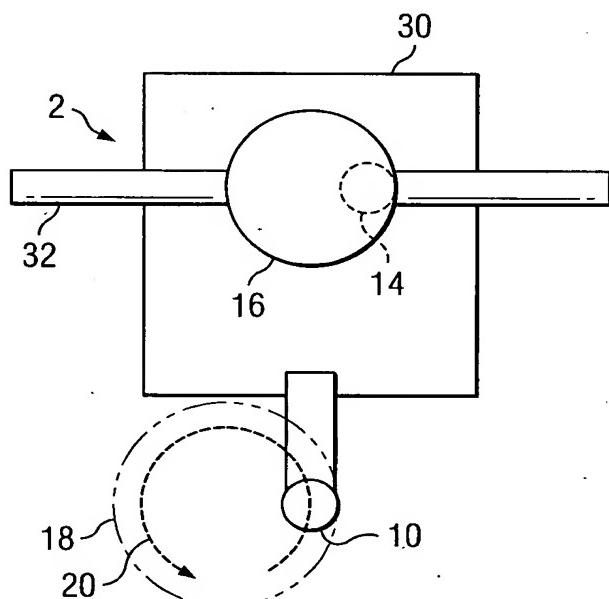


Fig. 10A



Fig. 9B




Fig. 10B

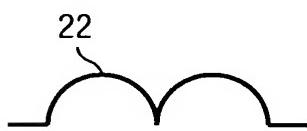


Fig. 9C



Fig. 10C

5/6

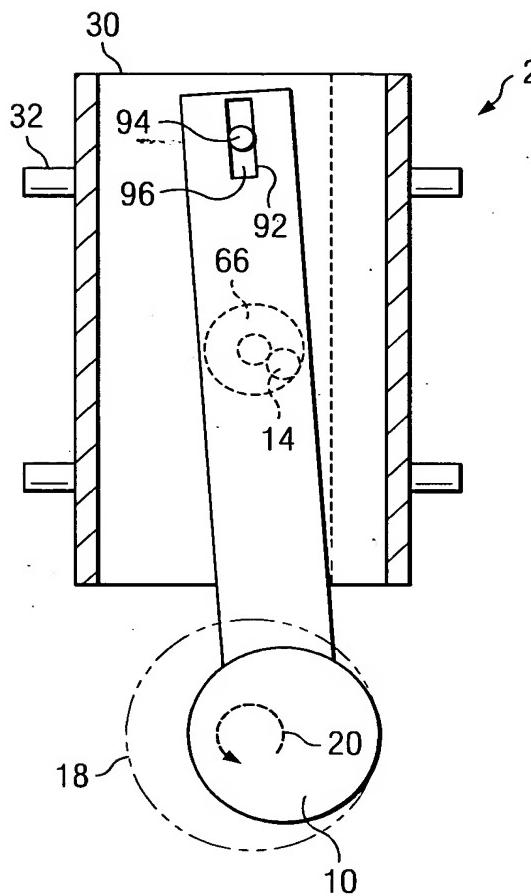


Fig. 11A

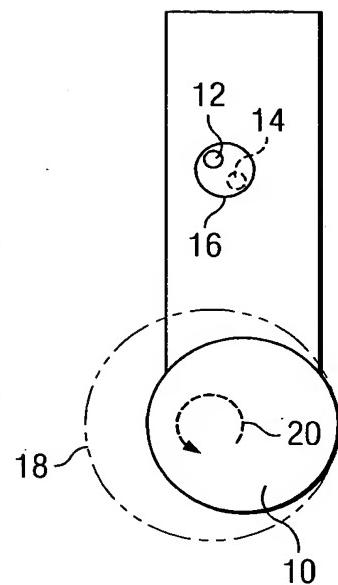


Fig. 12A



Fig. 11B



Fig. 12B

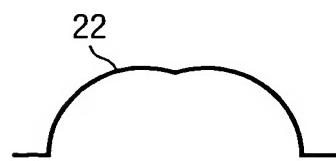


Fig. 11C



Fig. 12C

CIP of Serial No. 10/294,502 - 31132.165
Alex Kunzler
**BONE REMOVAL DEVICE AND METHOD
OF USE**

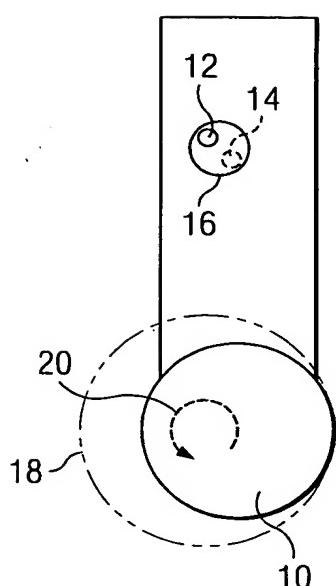


Fig. 13A



Fig. 13B



Fig. 13C

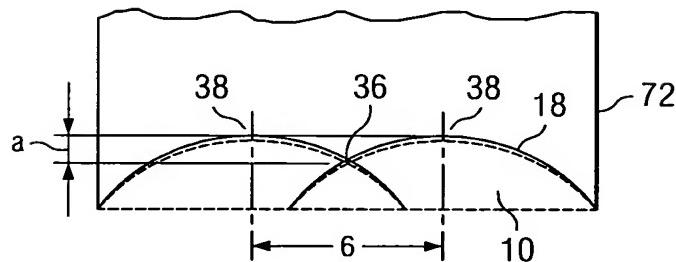


Fig. 14A

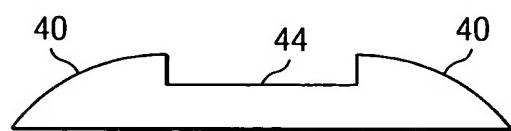


Fig. 14B

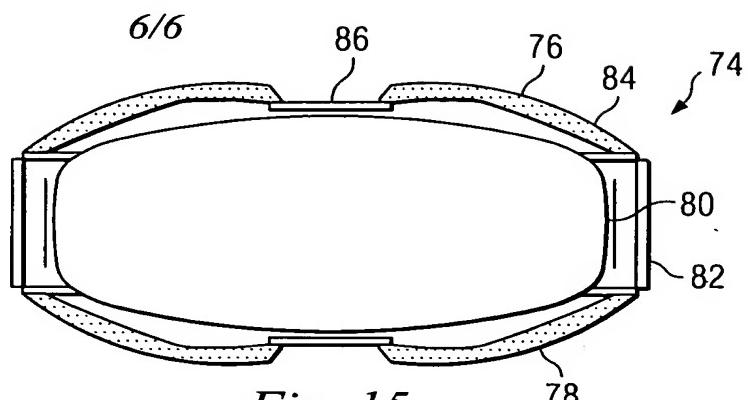


Fig. 15

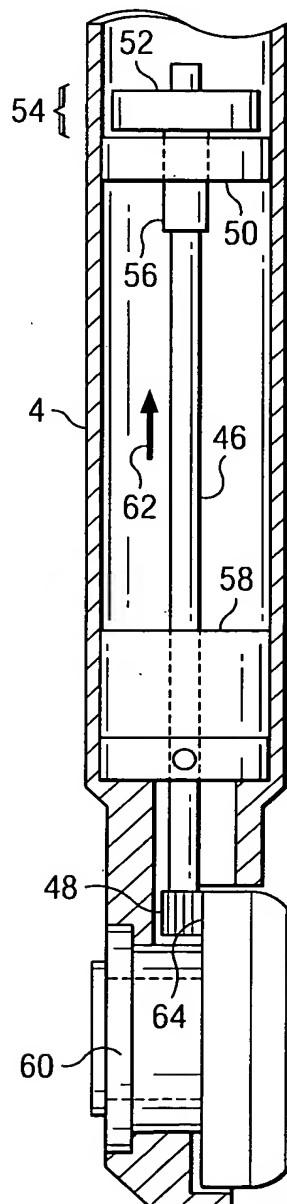


Fig. 16